


Sample Information

Acquired by : System Administrator
 Sample Name : GHK-Cu
 Tray# : 1
 Vial# : 3
 Injection Volume : 10
 Data File : 20240506-GHK-Cu(1-1,HAc)-240501.lcd
 Method File : GHK-Cu(0.1%TFA).lcm
 Batch File : 20240506-GHK-Cu .lcb
 Report Format File : DEFAULT.lsr
 Date Acquired : 5/6/2024 15:21:23
 Date Processed : 5/6/2024 15:58:03

Chromatogram

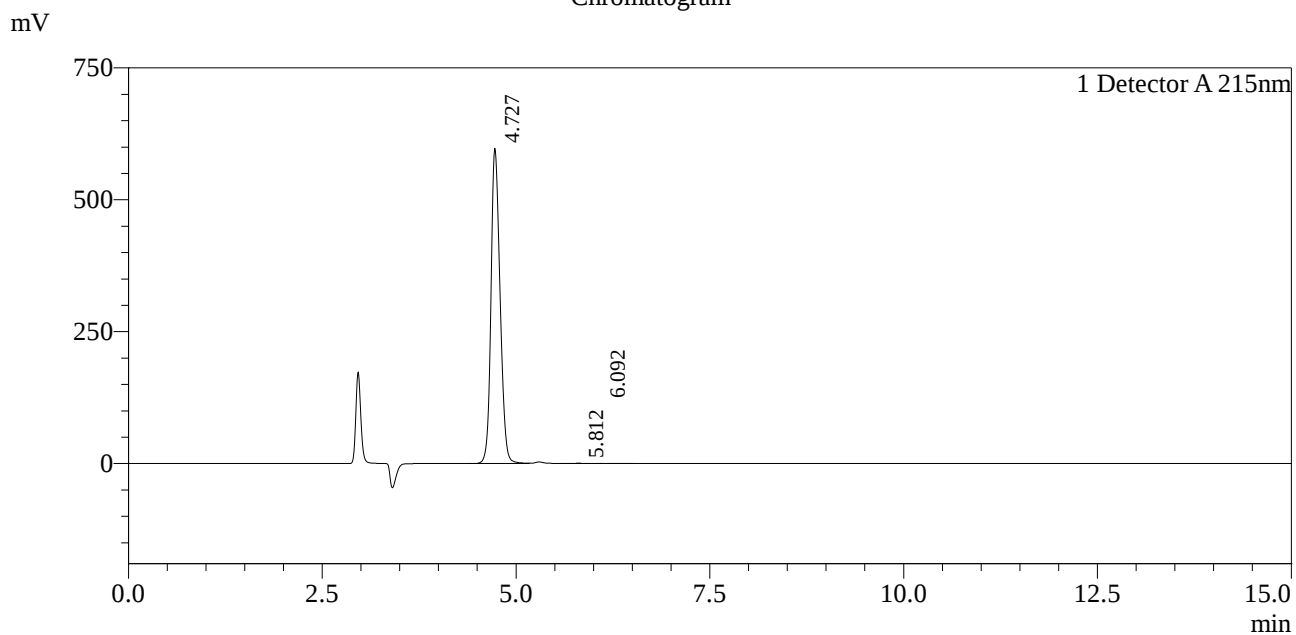

Peak Table

Detector A 215nm

Ret. Time	Area	Area%	Height	Width	Resolution	Tailing Factor	NTP
4.727	4904744	99.83	597600	0.225	--	1.179	7069
5.812	7591	0.15	385	0.585	2.679	--	1580
6.092	995	0.02	82	0.386	0.576	--	3994
	4913330	100.00	598067				